


PICO-500 Overview and Calibration

MICHAELA ROBERT, QUEEN'S UNIVERSITY

CAP CONGRESS - JUNE 2023


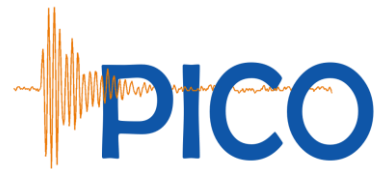


PICO Bubble Chambers

- Series of dark matter detectors operated at SNOLAB
- Aim to directly detect Weakly Interacting Massive Particles (WIMPs) via recoiling of target nuclei
- Cameras watch, piezoelectric transducers listen and pressure transducers feel for bubbles in superheated fluid





PICO Detectors

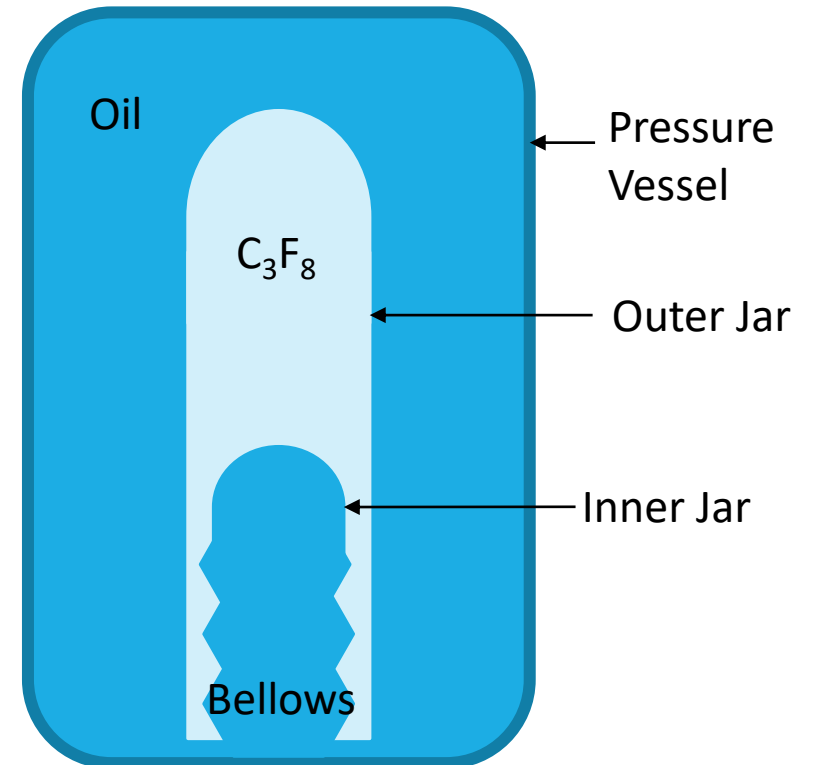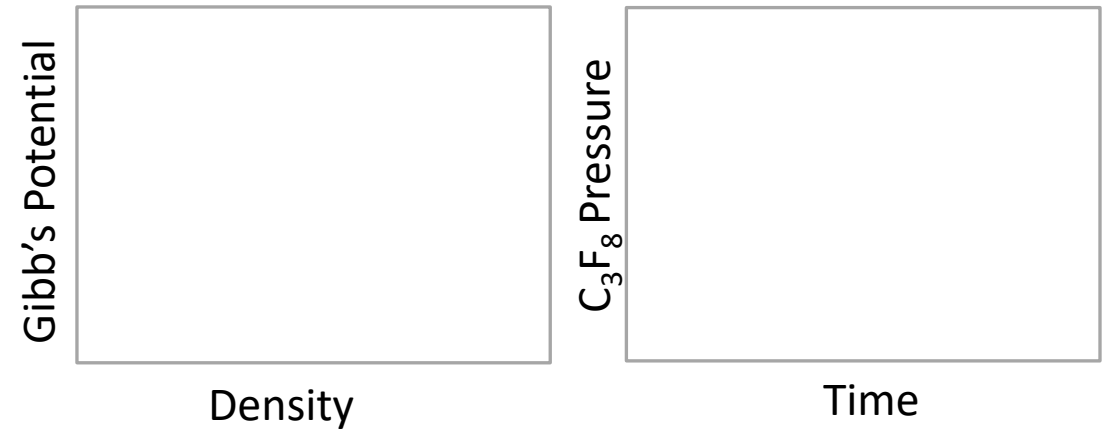



PICO Detectors

1. C_3F_8 is pressurized to stable liquid state

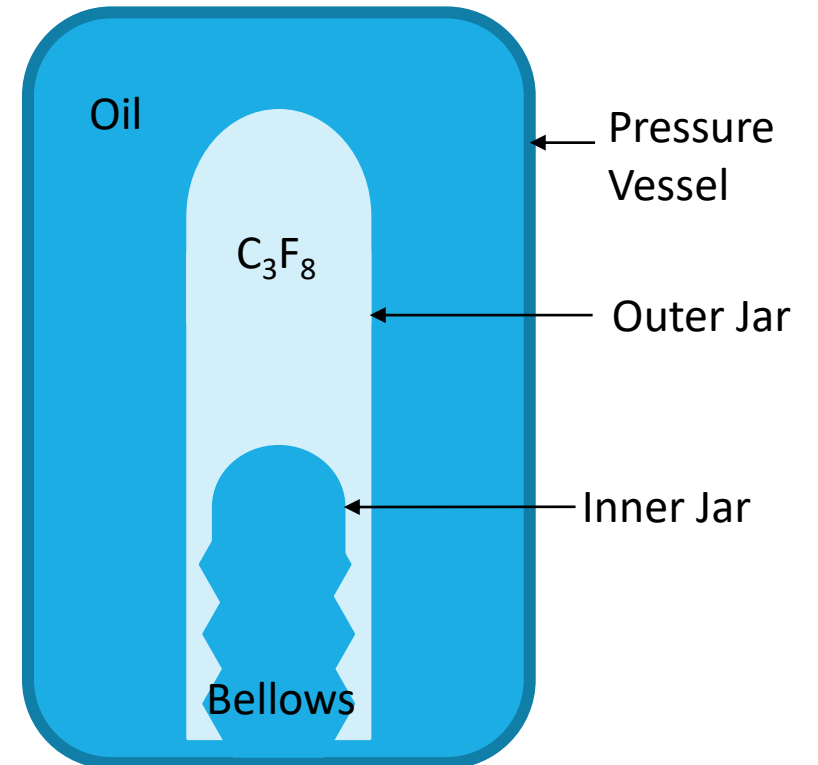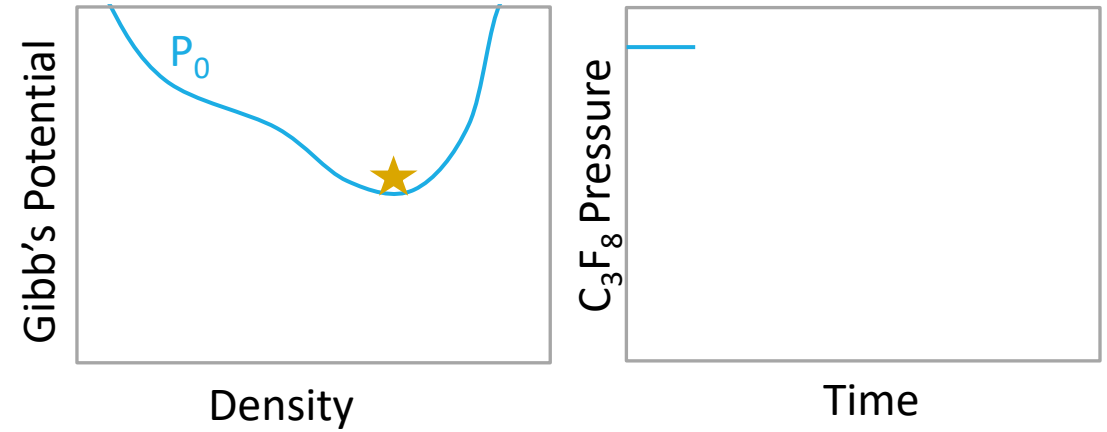



PICO Detectors

1. C_3F_8 is pressurized to stable liquid state
2. C_3F_8 volume is slowly expanded

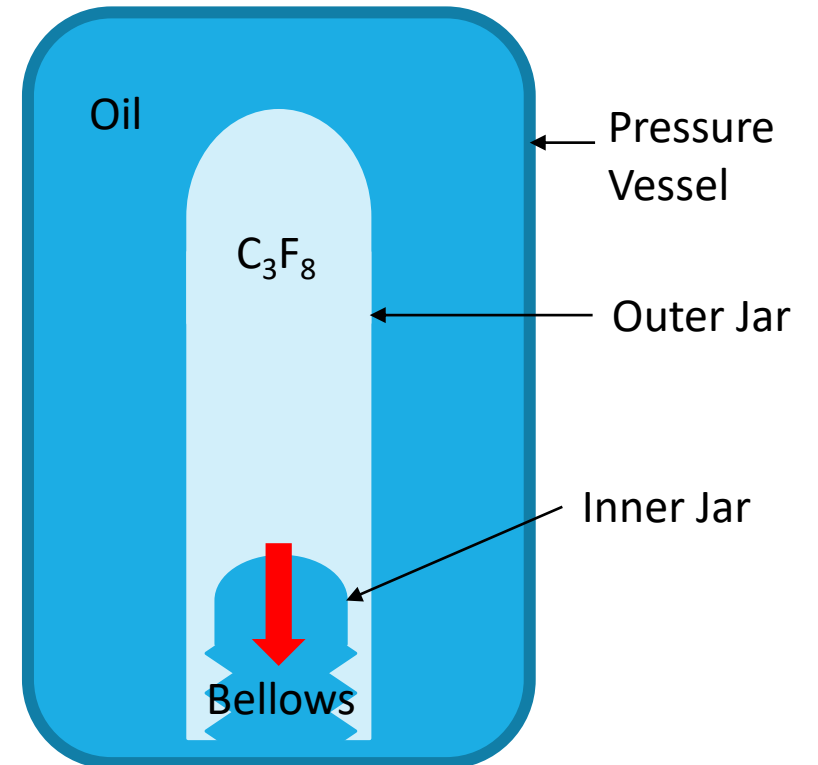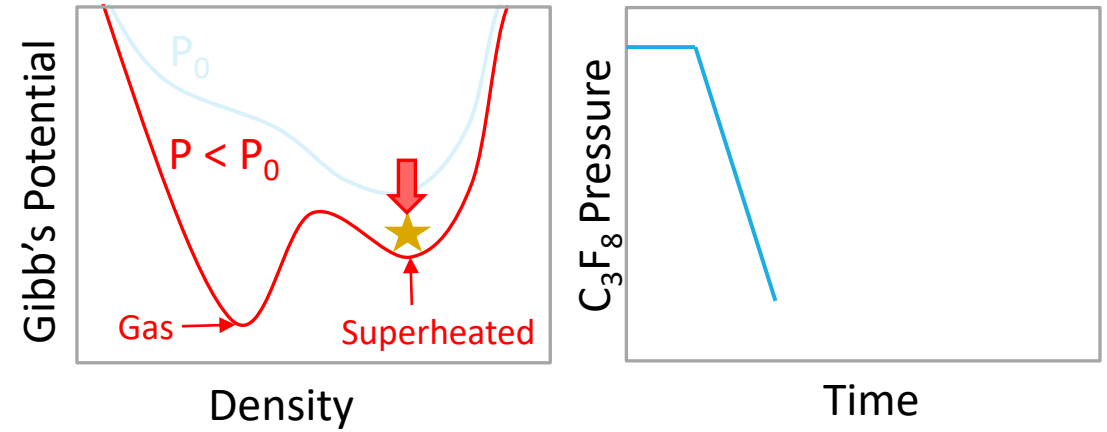



PICO Detectors

1. C_3F_8 is pressurized to stable liquid state
2. C_3F_8 volume is slowly expanded
3. Detector waits for a bubble in superheated state

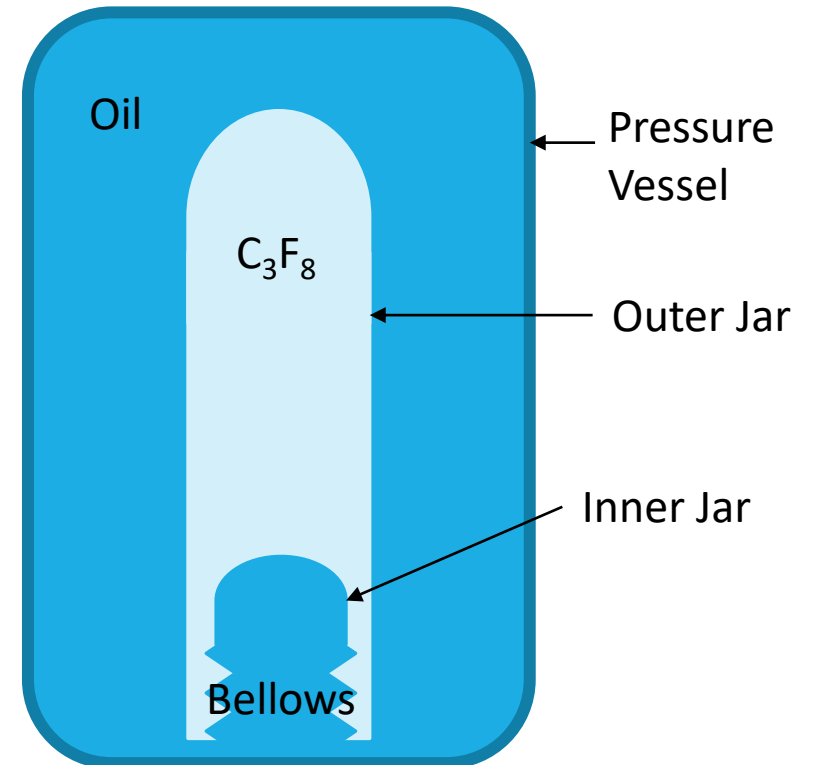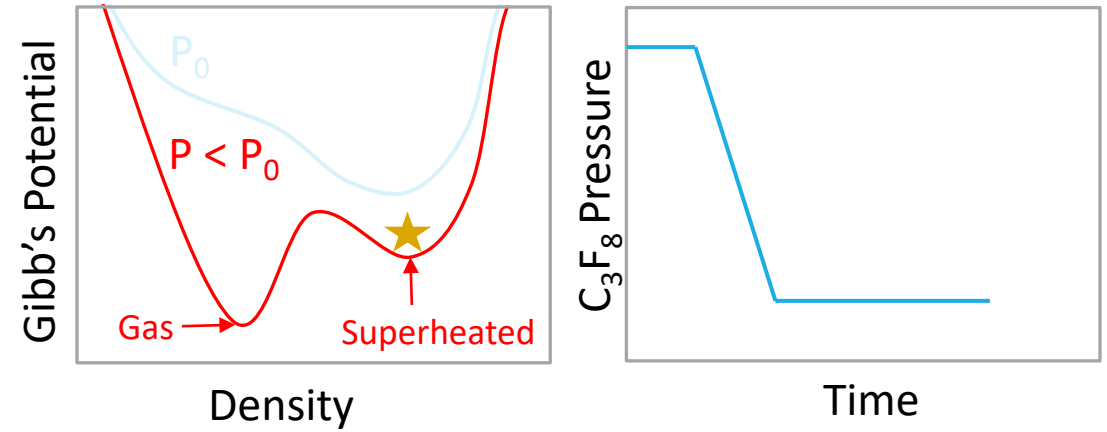



PICO Detectors

1. C_3F_8 is pressurized to stable liquid state
2. C_3F_8 volume is slowly expanded
3. Detector waits for a bubble in superheated state
4. Incoming particle causes a nuclear recoil resulting in a bubble - images, pressure and acoustic data are recorded

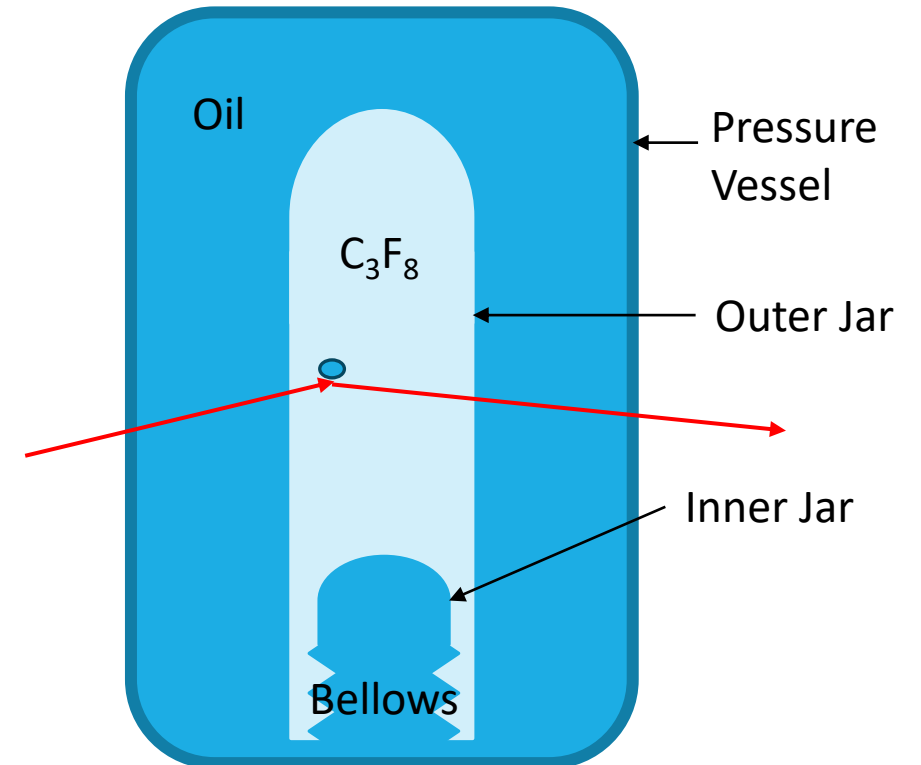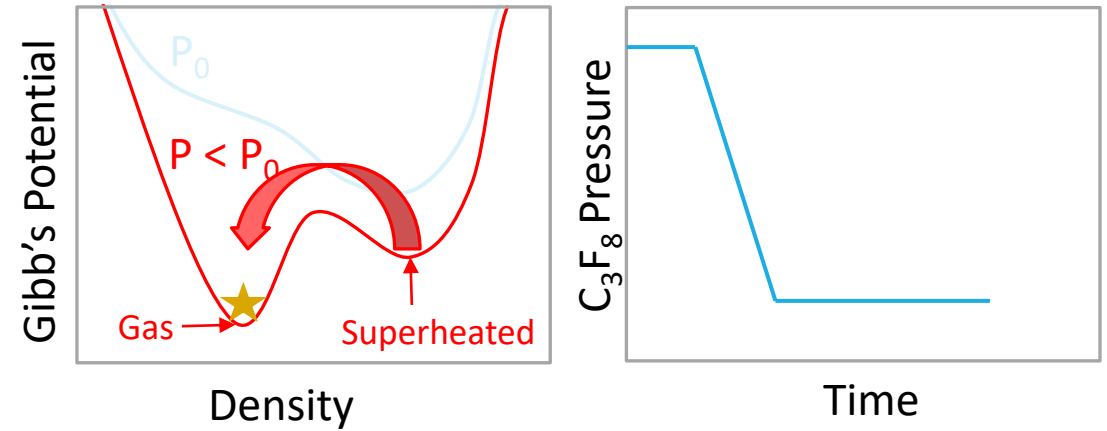

PICO Detectors

1. C_3F_8 is pressurized to stable liquid state
2. C_3F_8 volume is slowly expanded
3. Detector waits for a bubble in superheated state
4. Incoming particle causes a nuclear recoil resulting in a bubble - images, pressure and acoustic data are recorded
5. Detector compresses to collapse the bubble and reset for next event

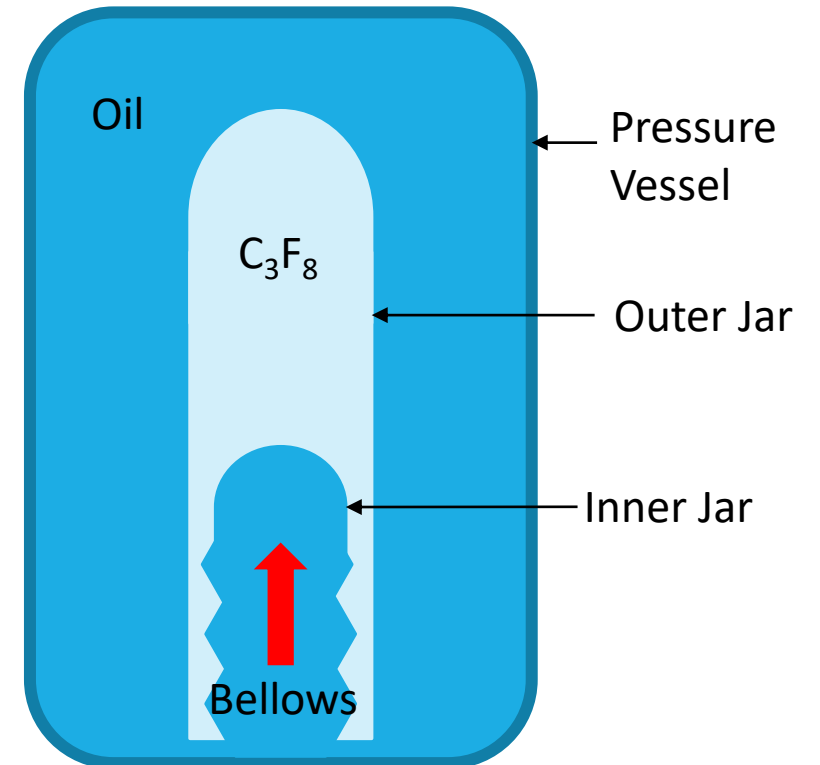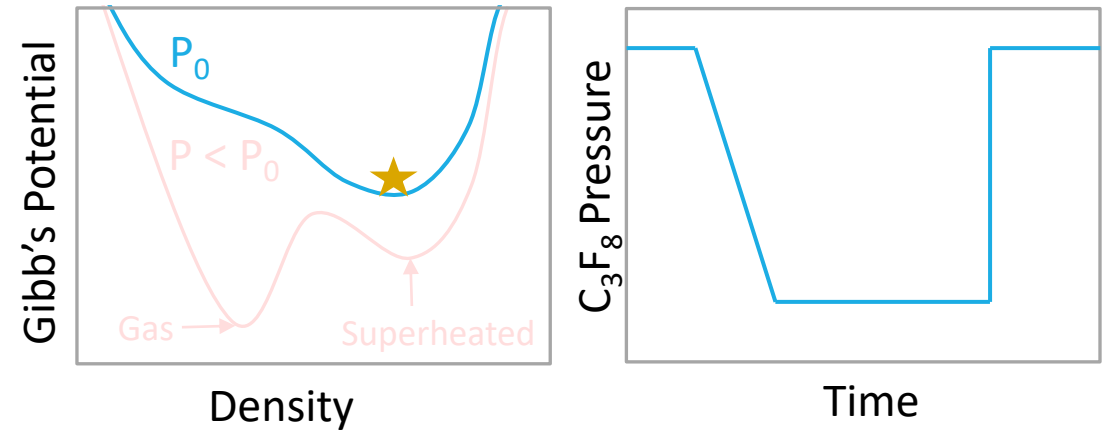

Detector Thresholds


- A small addition of energy, such as a nuclear recoil caused by a WIMP, can trigger a phase transition

- Seitz model: a bubble only sustains itself if the energy deposited within a local region surpasses an energy threshold

Typically ~ 25 nm



- PICO detectors can be set to ranges of expanded temperatures and pressures to reach various energy thresholds

Typically ~ 3 keV

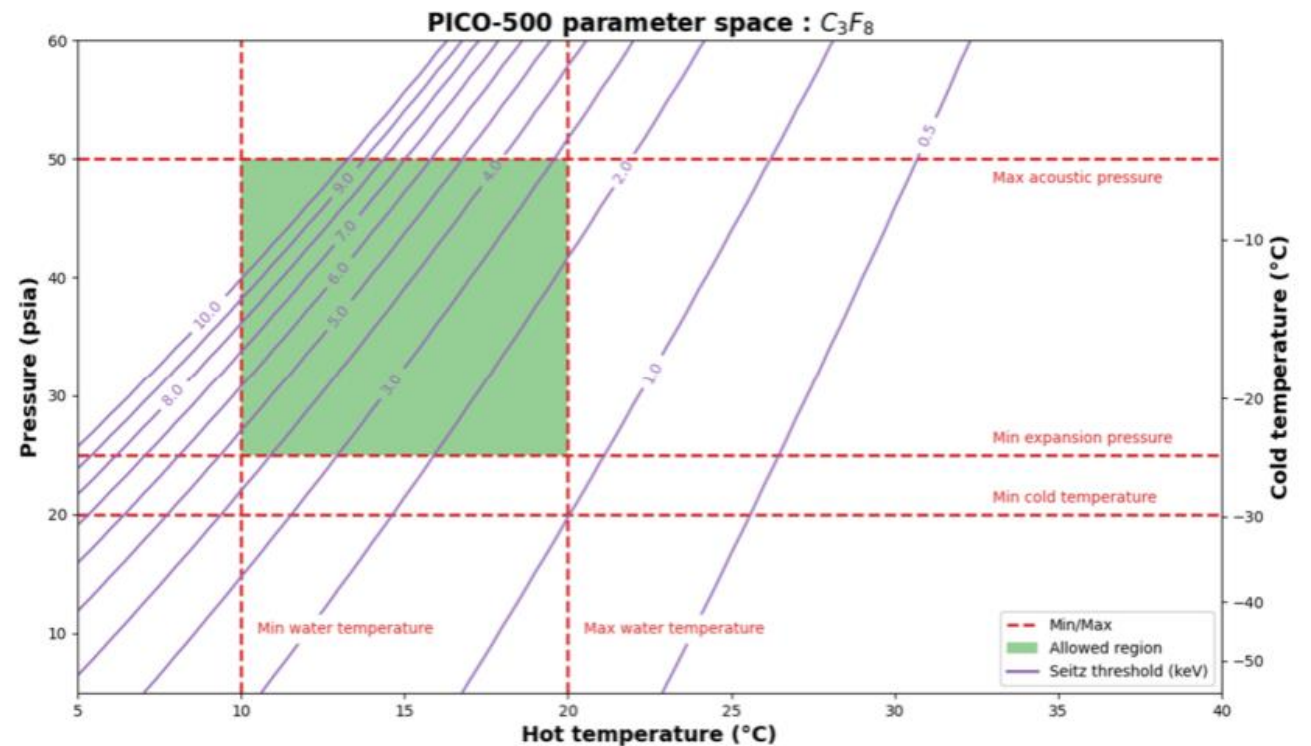


PICO-40L

- Constructed at SNOLAB between 2019-2023
- Currently in commissioning phase
- Projected 10 times improvement on spin-dependent WIMP sensitivity over PICO-60

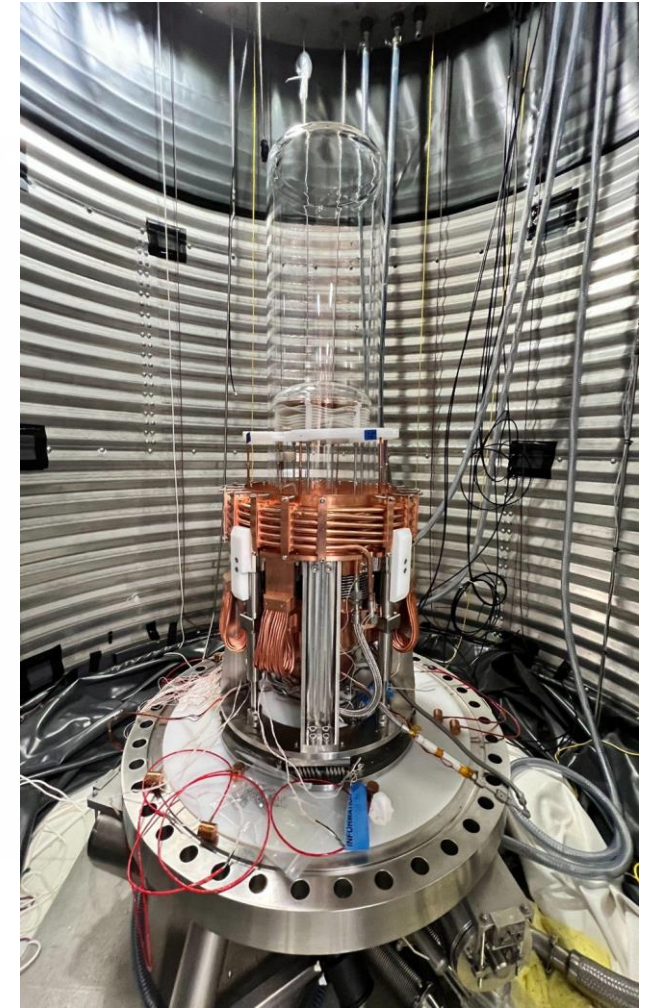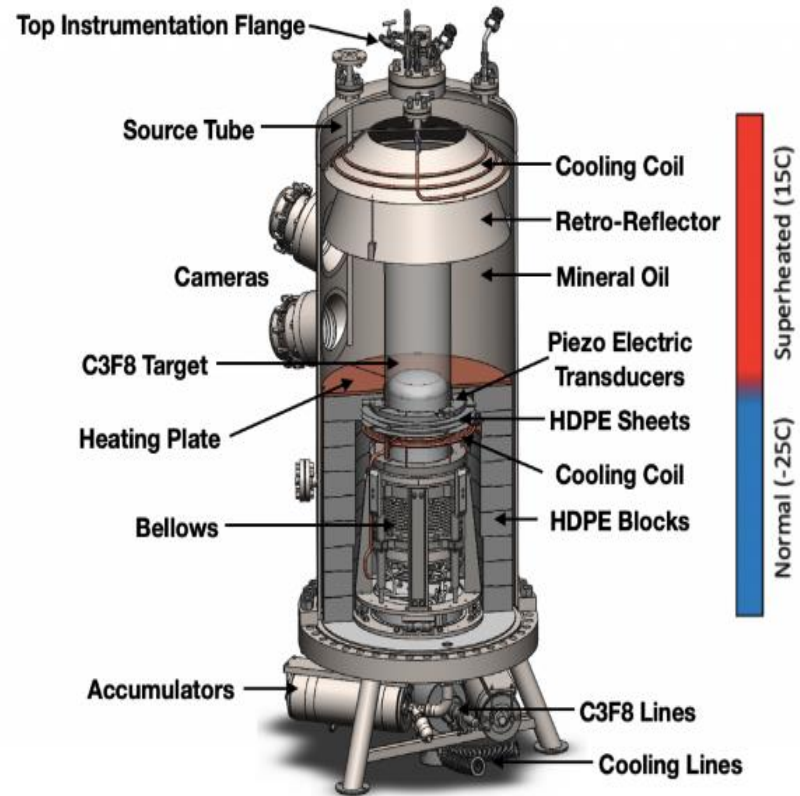


Upscaling to PICO-500

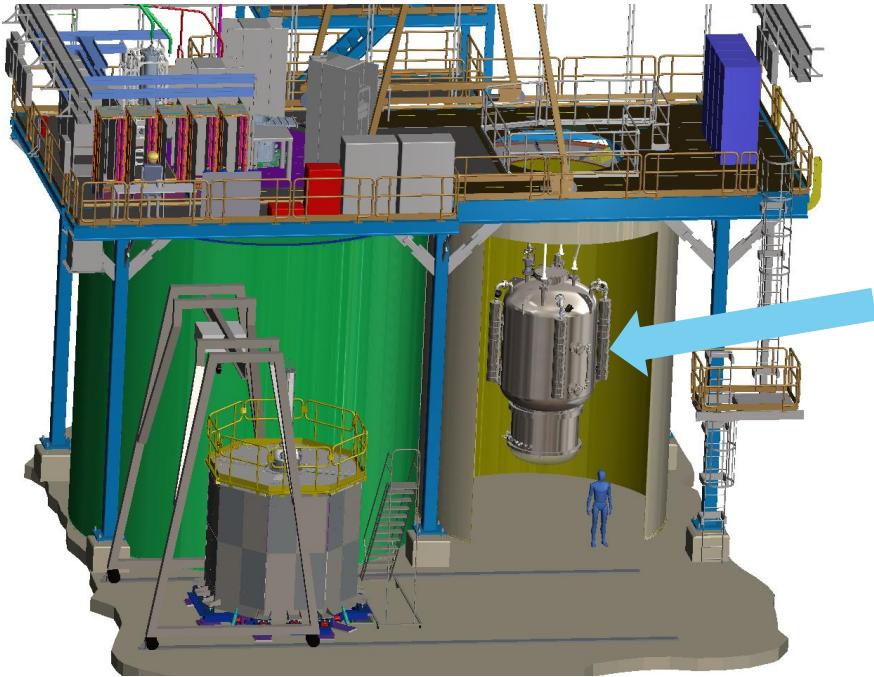

- ~250 litre sensitive volume (limited by available jars), 5 times larger than PICO-40L
- Upgrades to piezos, thermal system, and other systems
- 9000 kg pressure vessel
- To be suspended inside a 25 ft tall, 18.5 ft wide water tank
- To be constructed in Cube Hall at SNOLAB
- Fabrication of components has begun



PICO-500 Operation

- 1 month of initial calibration to begin in 2024
- 2 years of blind physics data in C_3F_8 at multiple thresholds
 - Low threshold run time limited by neutrino backgrounds
- Projected O(10) times improvement on spin-dependent WIMP sensitivity over PICO-40L
- Potential operation with other liquids:
 - CF_3I
 - CF_3CH_2F (R134a)
- Designed for future sensitive volume upsizing if larger vessels become available

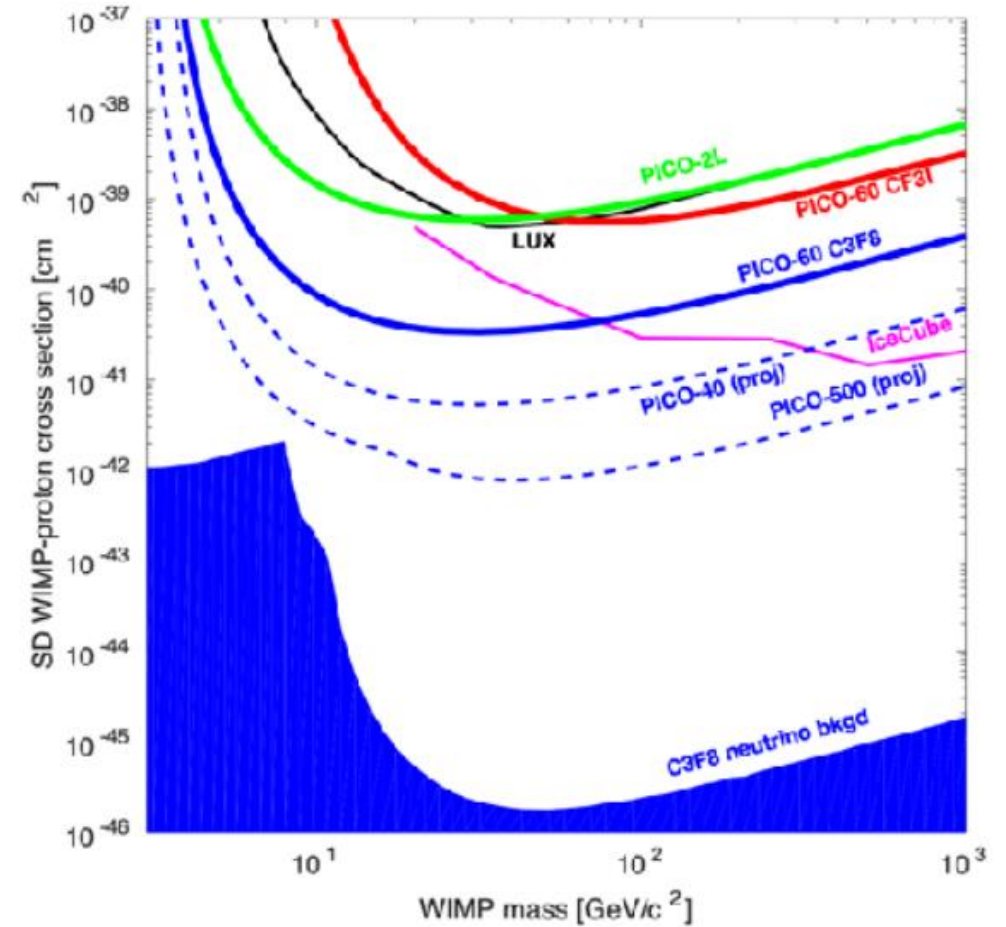



PICO-500 Calibration System

- Deploy calibration sources into the detector through source tubes
- Three source tubes at two different radii from C_3F_8 volume
- Monitor the position of the source for direct comparison of detector responses with simulation results
- Calibrate to establish detector response and stability, to reject backgrounds, etc.

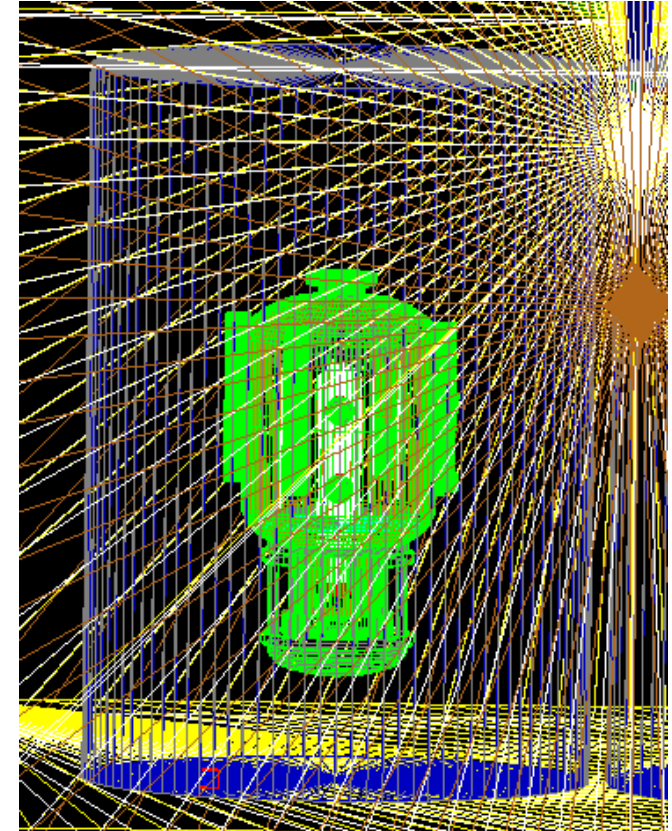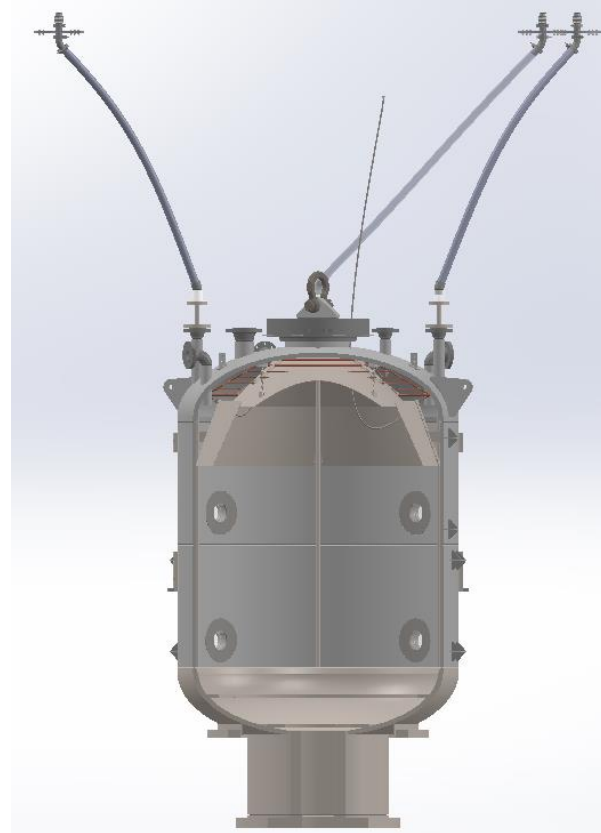

Calibrating for Alpha Rejection

- Alphas make louder bubbles than neutrons/WIMPs as recorded by piezoelectric sensors on outer jar
- Acoustic parameter (AP) describes the bubble's acoustic power
- $^{241}\text{AmBe}$ and/or ^{252}Cf calibration data is used to tune AP coefficients for neutron/WIMP – alpha separation

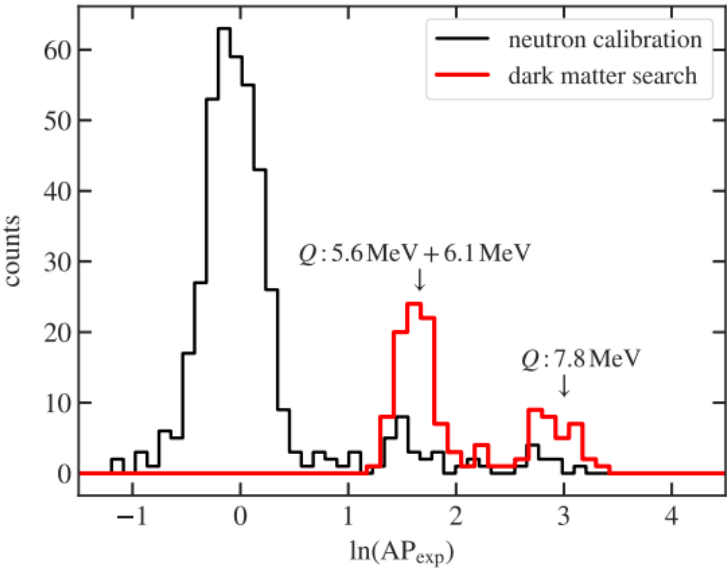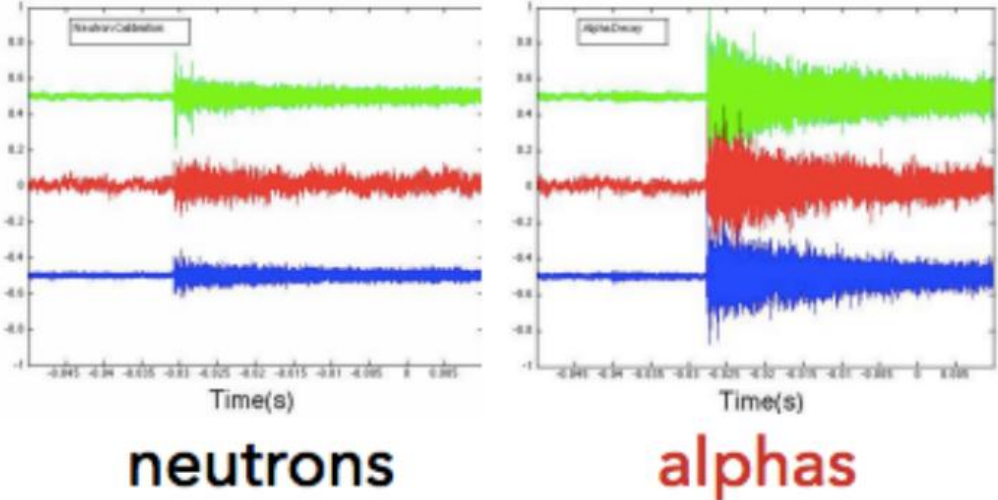

Tetiana Kozyrnets, Scott Fallows, and Carsten B. Krauss Phys. Rev. D 100, 052001 (2019)

Calibrating for Neutron Rejection


- Neutron MFP \sim cm \rightarrow single/multiple bubbles
- WIMPs interact rarely \rightarrow single bubble

Statistics are required to pull out WIMP signal!

- PICO-60 multiple to single bubble ratio was 3:1, but must be measured for PICO-500
- $O(1-100)$ neutron/s $^{241}\text{AmBe}$ and/or ^{252}Cf sources are required for optimal neutron calibration run time




PICO-40L: 20230304_3 83

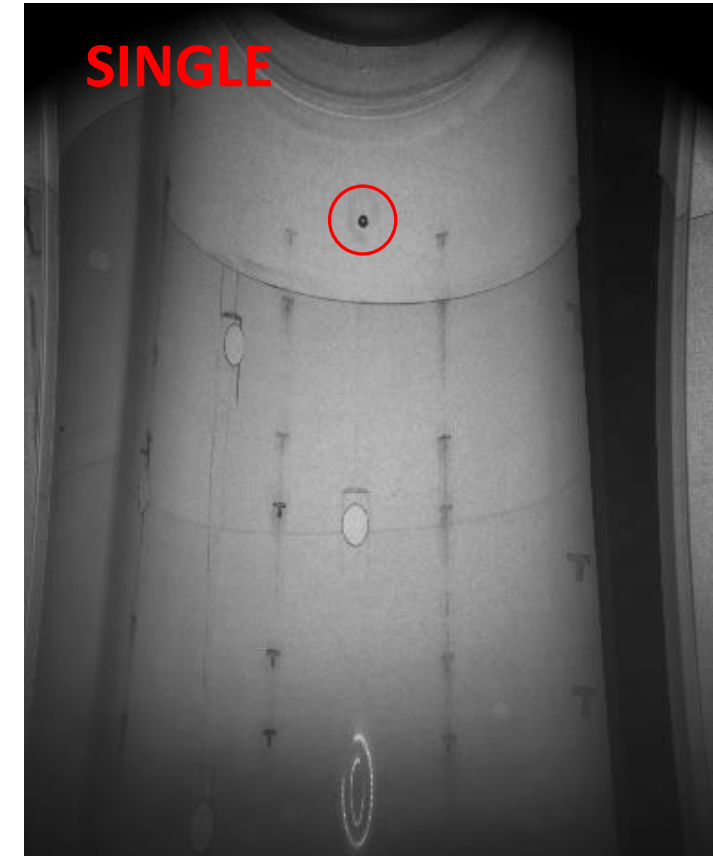

PICO-40L: 20230304_3 97

Calibrating for Gamma Rejection

- Electron stopping power is low \rightarrow rarely nucleate bubbles
- Objective to optimize threshold for WIMP sensitivity and gamma insensitivity
- ~ 18 MBq ^{60}Co source to probe detector response to electron recoils via 1.17 and 1.33 MeV gammas

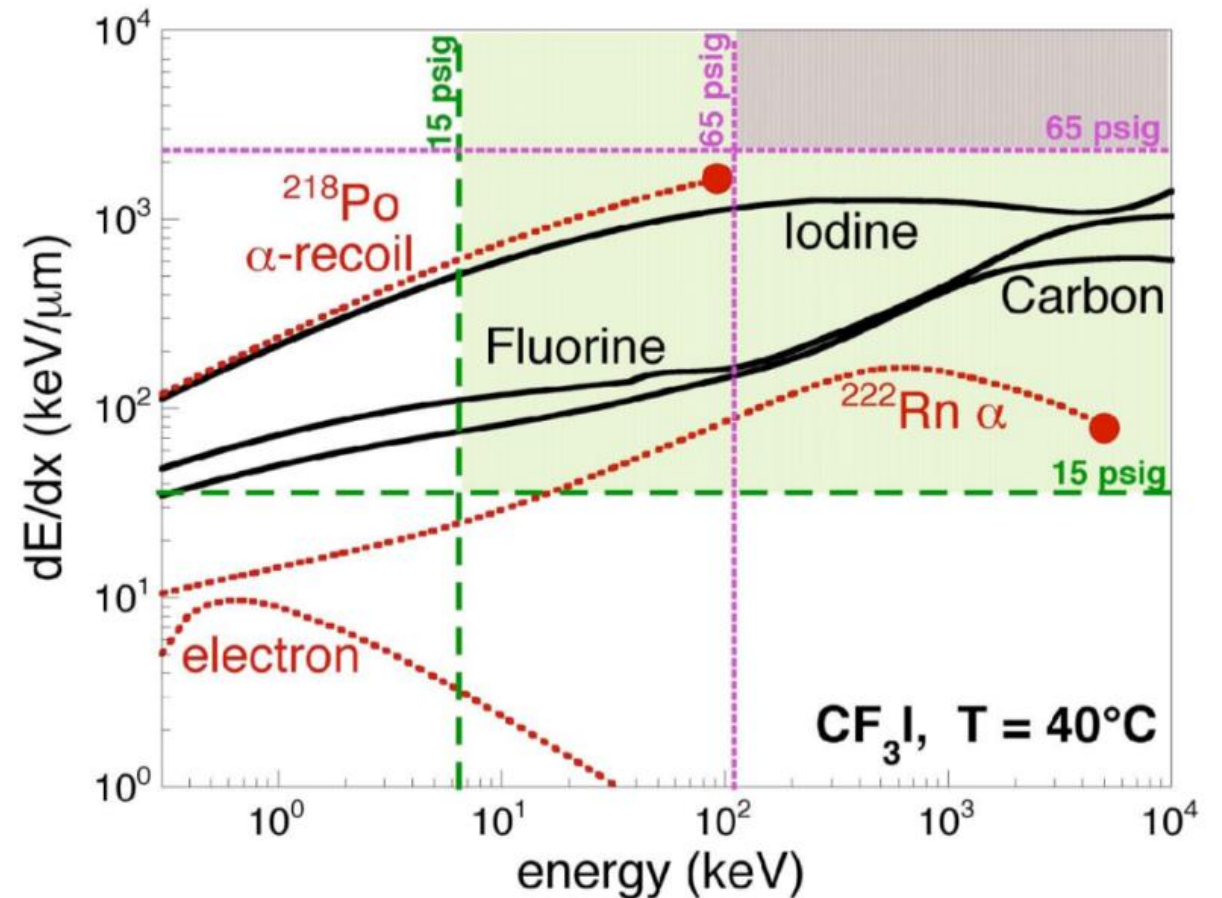


E. Behnke et al., Spin-Dependent WIMP Limits from a Bubble Chamber. *Science* 319, 933-936 (2008).
DOI: [10.1126/science.1149999](https://doi.org/10.1126/science.1149999)

Summary

- PICO-500 is projected to have world leading sensitivity to spin-dependent WIMP-proton interactions, improving on PICO-40L's sensitivity by $O(10)$
- Commissioning of PICO-500 is to start in 2024
- Calibrations for neutron statistics, alpha rejection, operating thresholds optimization, etc. are to be completed to achieve very low background rates



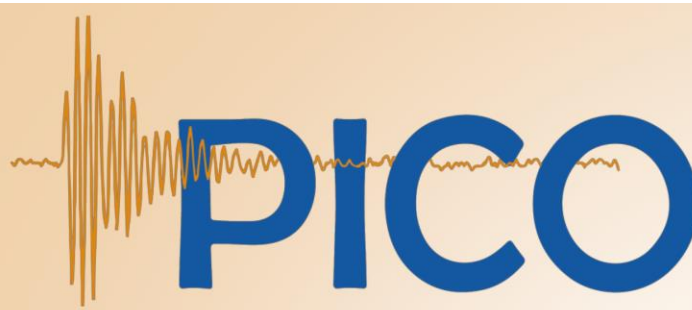


PICO



ČESKÉ
VYSOKÉ
UČENÍ
TECHNICKÉ
V PRAZE
R. Filgas, D. Mamedov,
E. Rukhadze, I. Stekl



PennState
D. Priya, S. Priya, Y. Yan



**NORTHWESTERN
UNIVERSITY**
C.E. Dahl



SNO+ LAB

P. Grylls, A. Mathewson,
I. Lawson, S. Sekula



**Northeastern
ILLINOIS UNIVERSITY**

O. Harris



Fermilab
P.S. Cooper, M. Crisler,
A. Sonnenschein



**Drexel
UNIVERSITY**
R. Neilson



IF
A. Acevedo-Rentería,
A. García-Viltres,
E. Vázquez-Jáuregui



J. Basu, M. Das,
V. Kumar

Thank you!



KICP

Kavli Institute
for Cosmological Physics
at The University of Chicago

J.I. Collar



**UNIVERSITY OF
ALBERTA**

M. Baker, S. Fallows,
C. Krauss, Q. Malin, S. Miller,
M. Rangen, C. Rethmeier,
P. Welingampola



**Pacific Northwest
NATIONAL LABORATORY**

I. Arnquist, C.M. Jackson,
B. Loer



**Queen's
UNIVERSITY**

E. Adams, M. Bai, K. Clark,
D. Cranshaw, K. Dering,
G. Giroux, H. Herrera,
C. Moore, A. Noble, M. Robert



**Université
de Montréal**

I. Brooklyn Varela, L. Desmarrais,
P. Frédérick, M. Laurin, V. Monette,
H. Nozard, A. Robinson, J. Savoie,
N. Starinski, V Zacek, C. Wen Chao



**Laurentian University
Université Laurentienne**

J. Farine, A. Le Blanc,
C. Licciardi, U. Wichoski



**INDIANA UNIVERSITY
SOUTH BEND**

E. Behnke, C. Cripe,
I. Levine,

Backup Slides

Seitz Threshold

$$E_T = \underbrace{4\pi r_c^2 \left(\sigma - T \frac{\partial \sigma}{\partial T} \right)}_{\text{Bubble surface}} + \underbrace{\frac{4\pi}{3} r_c^3 \rho_b (h_b - h_l)}_{\text{Latent heat of vaporization}} - \underbrace{\frac{4\pi}{3} r_c^3 (P_b - P_l)}_{\text{Double counted Work}}, \quad P_b - P_l \geq \frac{2\sigma}{r_c}$$

where,

E_T = Seitz threshold

r_c = critical bubble radius

T = temperature

ρ_b = bubble vapor density

h_i = specific enthalpy of bubble vapor (*b*) or superheated liquid (*l*)

P_i = Pressure in bubble (*b*) or superheated liquid (*l*)

σ = surface tension

Acoustic Parameter

$$AP = A(T) \sum_j G_j \sum_n C_n(\vec{x}) \sum_{f_{min}^n}^{f_{max}^n} f \times psd_f^j$$

Where,

$A(T)$ = scale factor

G_j = gain of j^{th} acoustic transducer


$C_n(\vec{x})$ = position dependence correction factor for n^{th} frequency bin

f = center frequency of n^{th} frequency bin

psd_f^j = power spectral density for n^{th} frequency bin and j^{th} acoustic transducer

Wall Events

- 4 cameras record images of bubbles, software reconstructs the bubble's location from the images
- Bubbles that nucleate near the walls of the jars are often alphas from the jars or wall events -> Bubbles outside of the fiducial volume are rejected
- $^{241}\text{AmBe}$ and/or ^{252}Cf neutron sources are chosen to induce bubbles at a desired rate

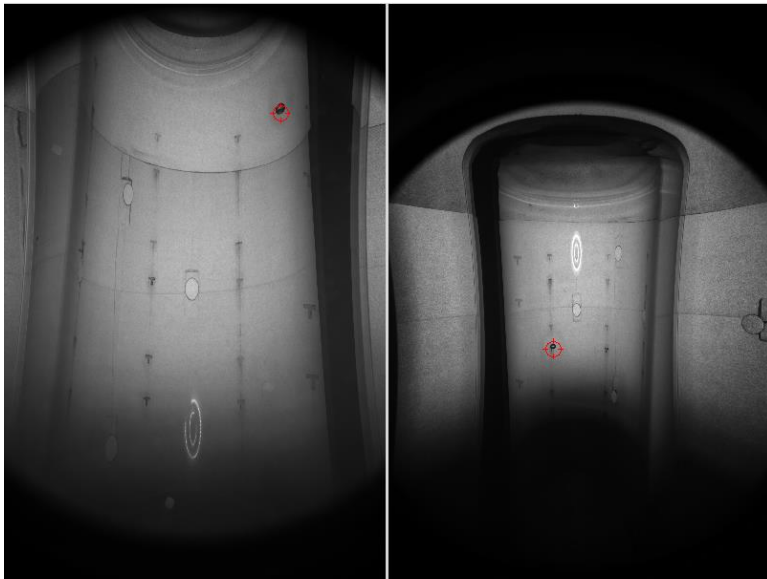

PICO-40L Event

